


Sample Name: UNKNOWN

```
=====  
Acq. Operator   : RolandNickyLauren  
Acq. Instrument : Homer                      Location : Vial 101  
Injection Date  : 11/3/2011 5:17:50 PM      Inj       : 1  
                                           Inj Volume : Manually  
  
Acq. Method     : C:\CHEM32\1\METHODS\HOMER QUANT ALC NOV 3.M  
Last changed    : 11/3/2011 5:17:10 PM by RolandNickyLauren  
                  (modified after loading)  
  
Analysis Method : C:\CHEM32\1\DATA\THE BEST.M  
Last changed    : 12/7/2011 8:25:43 PM  
                  (modified after loading)  
  
Sample Info     :
```

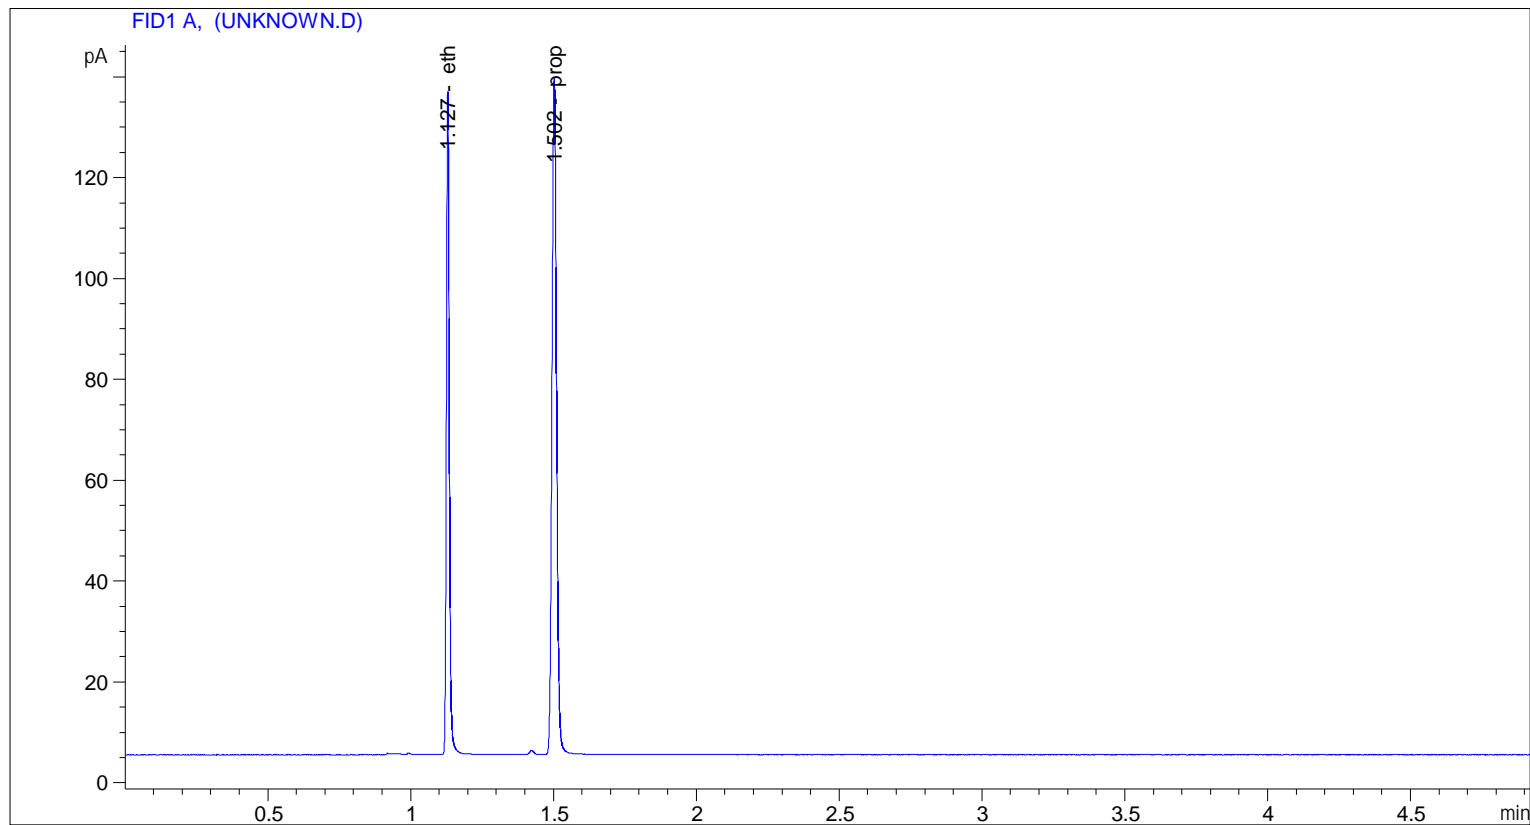

```
=====  
Internal Standard Report  
=====
```

```
Sorted By           : Signal  
Calib. Data Modified : 11/3/2011 5:52:09 PM  
Multiplier:         : 1.0000  
Dilution:           : 1.0000  
Do not use Multiplier & Dilution Factor with ISTDs  
Sample ISTD Information:  
ISTD ISTD Amount Name  
# [ng/ul]  
-----|-----|-----  
1 1.00000e-1 prop
```

Sample Name: UNKNOWN

Signal 1: FID1 A,

RetTime [min]	Type	ISTD used	Area [pA*s]	Amt/Area ratio	Amount [ng/ul]	Grp	Name
1.127	BB	1	92.57917	1.32575	1.88701e-1		eth
1.426		1	-	-	-		acet
1.502	BBA I	1	65.04339	1.00000	1.00000e-1		prop

Totals without ISTD(s) : 1.88701e-1

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

=====
*** End of Report ***