


Sample Name: UNKNOWN

```
=====  
Acq. Operator   : RolandNickyLauren  
Acq. Instrument : Homer                      Location : Vial 101  
Injection Date  : 11/3/2011 5:17:50 PM      Inj       : 1  
                                           Inj Volume : Manually  
  
Acq. Method     : C:\CHEM32\1\METHODS\HOMER QUANT ALC NOV 3.M  
Last changed    : 11/3/2011 5:17:10 PM by RolandNickyLauren  
                  (modified after loading)  
  
Analysis Method : C:\CHEM32\1\DATA\THE BEST.M  
Last changed    : 12/7/2011 8:24:35 PM  
                  (modified after loading)  
  
Sample Info     :
```

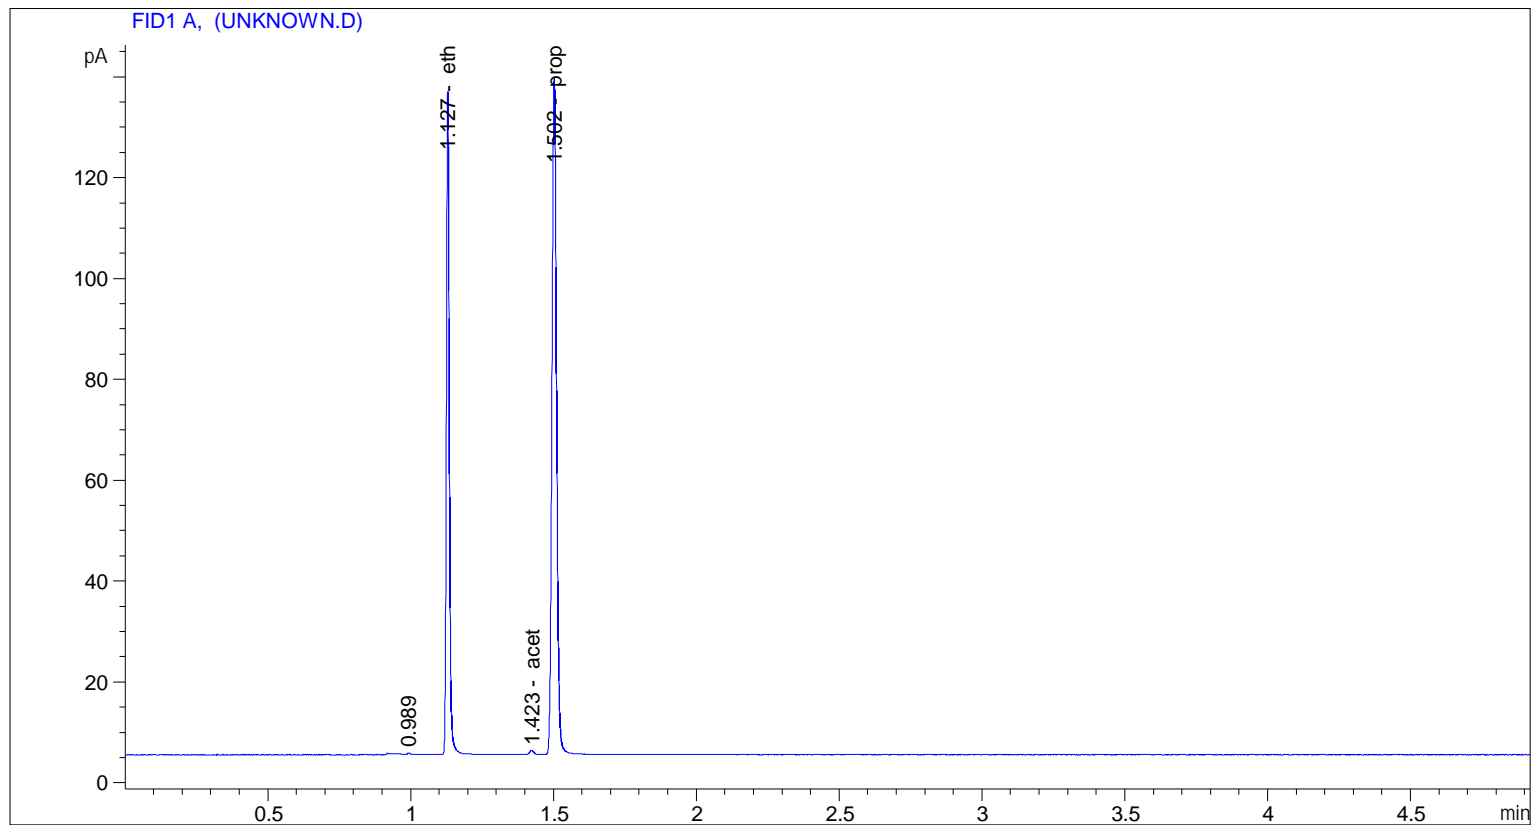

```
=====  
Internal Standard Report  
=====
```

```
Sorted By           :      Signal  
Calib. Data Modified :      11/3/2011 5:52:09 PM  
Multiplier:         :      1.0000  
Dilution:           :      1.0000  
Do not use Multiplier & Dilution Factor with ISTDs
```

Sample ISTD Information:

ISTD #	ISTD Amount [ng/ul]	Name
1	1.00000e-1	prop

Sample Name: UNKNOWN

Signal 1: FID1 A,

RetTime [min]	Type	ISTD used	Area [pA*s]	Amt/Area ratio	Amount [ng/ul]	Grp	Name
1.127	BB	1	92.57917	1.32575	1.88701e-1		eth
1.423	BB	1	8.44004e-1	0.00000	0.00000		acet
1.502	BBA	I 1	65.04339	1.00000	1.00000e-1		prop

Totals without ISTD(s) : 1.88701e-1

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Negative results set to zero (cal. curve intercept), (acet)

=====
*** End of Report ***