


Sample Name: UNKNOWN

```
=====
Acq. Operator   : RolandNickyLauren
Acq. Instrument : Homer                      Location : Vial 101
Injection Date  : 11/3/2011 5:17:50 PM      Inj       : 1
                                                Inj Volume: Manually

Acq. Method     : C:\CHEM32\1\METHODS\HOMER QUANT ALC NOV 3.M
Last changed    : 11/3/2011 5:17:10 PM by RolandNickyLauren
                  (modified after loading)

Analysis Method : C:\CHEM32\1\METHODS\THE BEST.M
Last changed    : 1/19/2013 10:14:57 AM
                  (modified after loading)

Sample Info     :
```

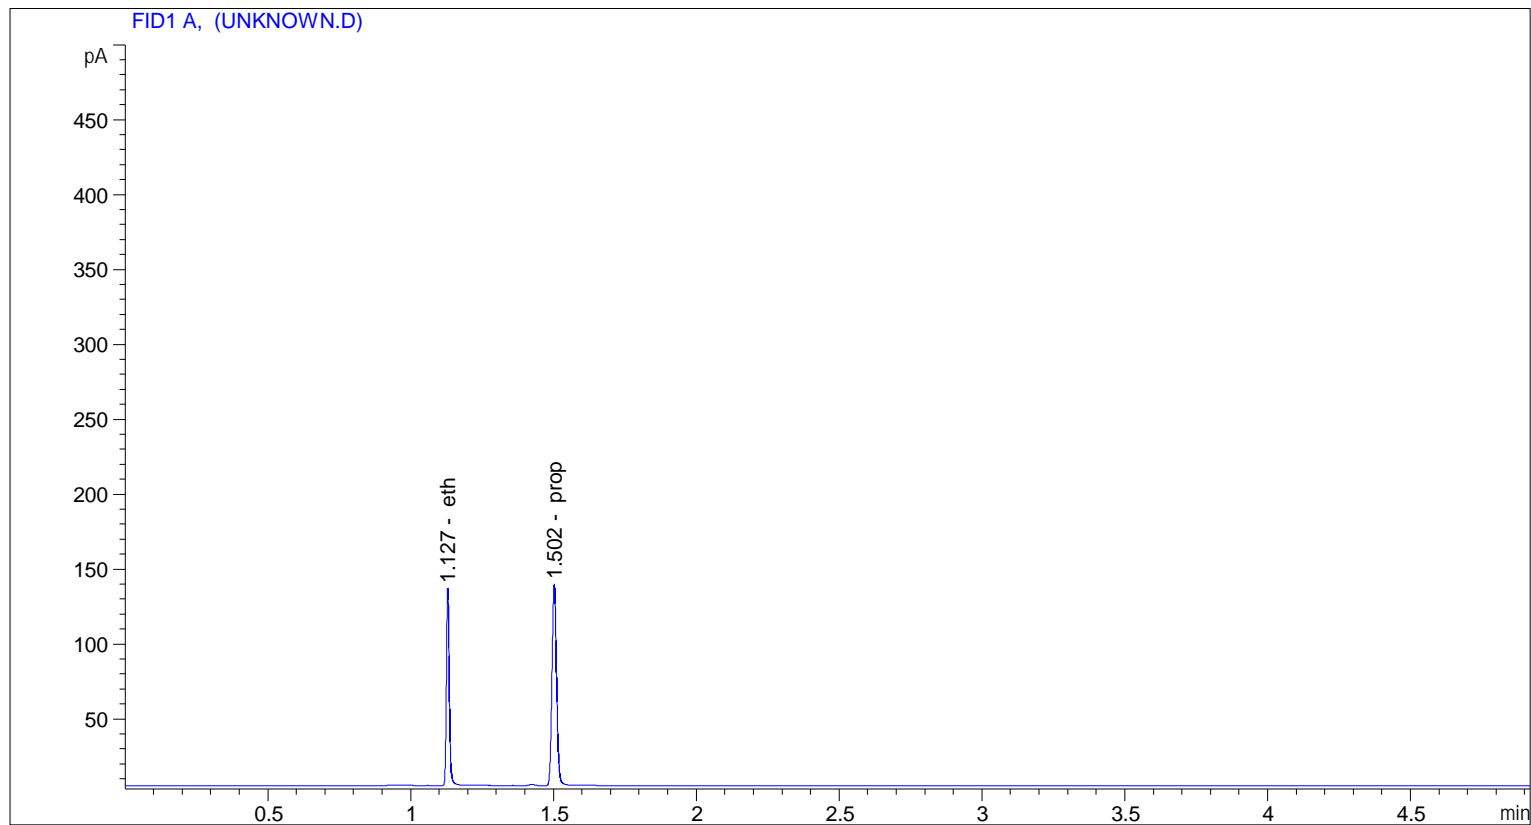

```
=====
Internal Standard Report
=====
```

```
Sorted By           : Signal
Calib. Data Modified : 11/3/2011 5:52:09 PM
Multiplier:         : 1.0000
Dilution:           : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Sample ISTD Information:

ISTD #	ISTD Amount [ng/ul]	Name
1	1.00000e-1	prop

Sample Name: UNKNOWN

Signal 1: FID1 A,

RetTime [min]	Type	ISTD used	Area [pA*s]	Amt/Area ratio	Amount [ng/ul]	Grp	Name
1.127	BB	1	92.57917	1.31874	1.67795e-1		eth
1.426		1	-	-	-		acet
1.502	BBA I	1	72.76004	1.00000	1.00000e-1		prop

Totals without ISTD(s) : 1.67795e-1

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

=====
*** End of Report ***